

Atom

The Journal of Laryngology and Otology

EDITED BY
G. H. BATEMAN

ASSISTANT EDITOR
LIONEL TAYLOR

Contents

The diagnosis and treatment of active cochlear otosclerosis	GEORGE E. SHAMBAUGH, JR.	301
Experimental middle ear homografts	R. S. DAWKINS	315
The fate of transplanted ossicles	A. G. KERR and G. D. L. SMYTH	337
Ethnic factors in the pathogenesis of chronic otitis media in Israel	J. SADÉ, S. KONAR and R. HINCHCLIFFE	349
The clinical significance of 'directional preponderance' concluded by electronystagmography	ABRAHAM EVIATAR and SYLVIA WASSERTHEIL	355
An objective study of the effect of Betahistine Hydrochloride on hearing and vestibular <i>Sete.</i> function tests in patients with Ménière's disease	T. J. WILMOT	369 ✓
The threshold of hearing in school children	J. M. A. LENIHAN, J. FULTON CHRISTIE, T. S. RUSSELL, N. M. ORR, MARGARET D. HAMILTON and ELIZABETH C. KNOX	375 ✓
Closure of antro-alveolar fistulae	HOLGER JUSELIUS and KALEVI KALTIOKALLIO	387 ✓
Clinical records—		
Tracheal stenosis	P. M. STELL	395 ✓
Cholesteatoma of maxillary sinus	S. K. DAS	397 ✓
Proboscis	G. DASGUPTA, S. K. KACKER and A. K. BHAN	401
Olfactory neuroblastoma	R. E. VAKIL and V. P. VAISHNAV	407
Hypoparathyroidism presenting as dysphagia	R. PALAT	411
Societies' proceedings		413
General notes		415

Headley Brothers Ltd
Ashford, Kent

Annual Subscription £8 net, U.S.A. \$23 Monthly, £1 net, post free

The Journal of Laryngology and Otology

(FOUNDED in 1887 by MORELL MACKENZIE and NORRIS WOLFENDEN)

EDITED BY

G. H. BATEMAN

ASSISTANT EDITOR

LIONEL TAYLOR

1. Original articles which have not been published elsewhere are invited and should be sent to the Editor. They are considered for publication on the understanding that they are contributed to this *Journal* solely. Reproduction elsewhere, in whole or in part, is not permitted without the previous written consent of the Author and Editor and the customary acknowledgement must be made.

2. Manuscripts should be typewritten, on one side only of the paper, and well spaced. Captions to illustrations should be typed on a separate sheet and sent at the same time as original photographs, etc.

The Harvard system of recording references should be used, e.g. GREEN, C., and BROWN, D. (1951), *Journal of Laryngology and Otology*, 65, 33. The titles of all Journals should be given without abbreviation.

It is most important that authors should verify personally the accuracy of every reference before submitting a paper for publication.

3. Galley proofs and engraver's proofs of illustrations are sent to the author. Corrections, which should be kept to a minimum, must be clearly marked, and no extra matter added. Proofs should be returned within 5 days.

4. Illustration blocks will normally be held by the Printers for three years, after which they will be destroyed. Any author is entitled to have these returned to him, but a request for this must be sent within three years of the appearance of the article, to HEADLEY BROTHERS LTD., The Invicta Press, Ashford, Kent. Coloured illustrations will be charged to authors, unless a special grant is authorized by the Editor.

5. Orders for reprints must be sent when returning galley proofs, and for this purpose special forms are supplied.

6. Editorial communications may be addressed to THE EDITOR, *Journal of Laryngology*, c/o HEADLEY BROTHERS LTD., The Invicta Press, Ashford, Kent.

7. The annual subscription is £8 (eight pounds sterling) post free; U.S.A. \$23 post free, and payable in advance.

8. Single copies of current or back numbers (when available) will be on sale at £1 (including postage) each.


9. All subscriptions, advertising and business communications should be sent to the publishers, or subscription agents.

HEADLEY BROTHERS LTD.

The Invicta Press, ASHFORD, Kent.

© *Journal of Laryngology and Otology Ltd.*, 1971

Thought reader!!

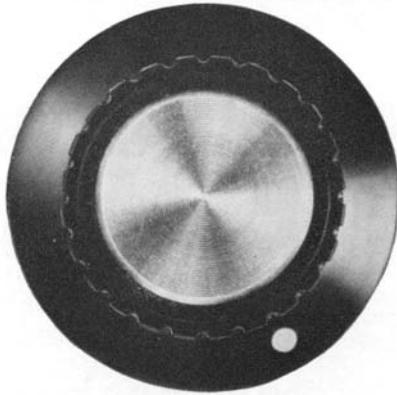

With the complex tests that are being done today clinical audiometry can become altogether too complicated.

By switching only one knob, the model 103 Clinical Audiometer will do the thinking for you, and enable you to select up to 18 different functions:

- Pure Tone Air Conduction
- Pure Tone Bone Conduction
- Narrow Band Masking
- Wide Band (White Noise) Masking
- Alternative Binaural Loudness Balance
- Simultaneous Binaural Loudness Balance
- Speech, Live Voice
- Speech, Recorded
- Speech with Masking
- SISI Test
- Luscher DL Test
- Audiometer Weber Test
- SAL Test
- Rainville Test
- Shifting Voice
- Stenger Test
- Modified Stenger Test
- Tone Decay Test

The model 103 is functional engineering with the operator in mind. We believe the audiometer should do the thinking ... and this one does just that.

To: Amplivox Hearing Conservation Ltd.,
 Beresford Avenue, Wembley, Middlesex.
 Tel: 01-902 8991

Name _____

Address _____

- Please send demonstrator
- Please send leaflet

JLO 4/71



the complete de-bugging device

clears both fungi and bacteria in ear infections

Candida albicans and *Aspergillus niger* are isolated in over 20 per cent of cases of otitis externa, and if high success rates are to be achieved treatment must take account of this. Otoseptil® ear drops employs a very broad-spectrum attack with efficient anti-inflammatory action.

The new antibiotic ester—neomycin undecylenate—provides potent dual bactericidal and antifungal activity.

Tryrothricin (containing gramicidin and tyrocin) effectively eliminates resistant Gram-positive cocci, while Hydrocortisone alcohol exerts its characteristic anti-inflammatory action. Rapid tissue contact is ensured by the penetrant Ethylene oxide polyoxypropylene glycol condensate, which is incorporated in the clear liquid ear drop.

For pain relief, AUDAX® ear drops may be used concomitantly with Otoseptil® ear drops because they are completely miscible and compatible.

Full information is available on request.

® Registered trade marks

Otoseptil

ear drops



Napp Laboratories Limited,
Watford WD2 7RA England



Please mention *The Journal of Laryngology and Otology* when replying to advertisements

In hospital and after...

Floxapen

simplifies antibiotic treatment

Floxapen, like Orbenin* (cloxacillin B.P.), is active against virtually all staphylococci, streptococci and pneumococci, irrespective of their sensitivity to other antibiotics. However, it is simpler to use than Orbenin, the established first-line treatment for Gram-positive infections in hospitals, because:


The standard dose, orally or by injection, is only 250 mg. q.i.d.

Equivalent serum levels are obtained by either route.

Transfer from injectable to oral therapy may be justified at an earlier stage of treatment.

Floxapen also offers the penicillin advantages of low toxicity and bactericidal action.

For outpatient treatment, Floxapen is ideal; its simple oral dosage and minimal side-effects encourage patients to follow the correct dosage and to complete the course of therapy.

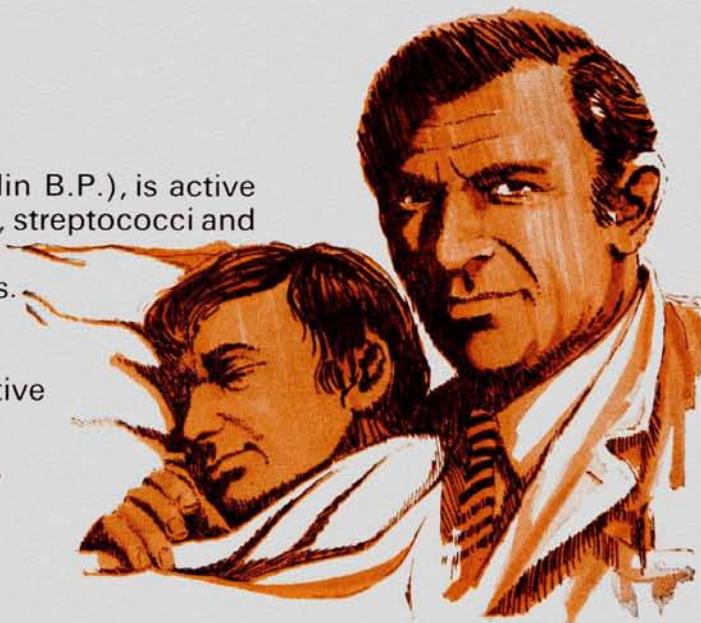

Indications: Infections due to sensitive Gram-positive organisms.

Dosage: Oral and Intramuscular:
Adults: 250 mg. q.i.d.
Children: 2-10 years—half adult dose;
Under 2 years—quarter adult dose.

Oral doses should be taken one hour before meals. In severe infections dosages may be increased if required.

Availability: Capsules (black/caramel) and Vials, each containing 250 mg. flucloxacillin.

Contra-indications: Penicillin hypersensitivity. Subconjunctival injection.

Side-effects: As with other penicillins.

Further information is available on request.

Floxapen

simplifies antibiotic treatment
flucloxacillin



Floxapen* (flucloxacillin) is a product of British research at

Beecham Research Laboratories, Brentford, England

<http://www.beecham.com> originators of the new penicillins Cambridge University Press

*regd





P. C. WERTH LTD. Contractors to H.M. Government
and Local Authorities
*Specialist Supply, Maintenance, Calibration Services for Audiological
Test and Teaching Equipment*

17 STRATFORD PLACE, OXFORD ST., LONDON W1N 0DH

Telephone: 01-629 5559

*Clinical, Diagnostic, Screening and Bekesy Audiometers. Acoustic Impedance Apparatus.
Stereo Auditory Trainers. Acoustic Cabins. Artificial Mastoid, etc.*

Kamplex DA11 Twin-Channel Clinical Audiometer

Our latest model with
many new features:


Probably the most keenly
priced twin-channel audio-
meter currently available.

Fowler, Sisi, Luscher and
Rainville test facilities
inbuilt.

Complete speech facilities.

Narrow band and white
noise masking to 100 db.

Pure tone attenuation to
120 db.

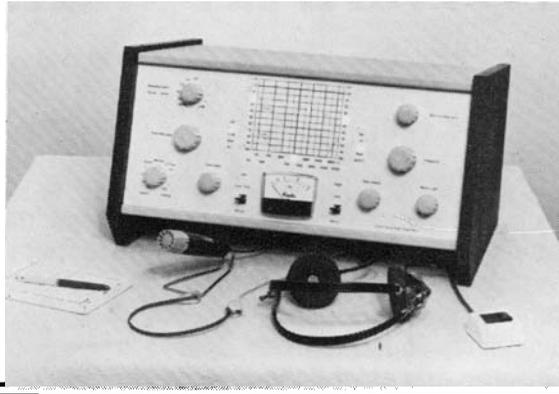

THE LARYNGOSCOPE

A Monthly Journal
devoted to the disease of
EAR, NOSE AND THROAT

*Official organ for the American Laryngological
Rhinological and Otological Society*


Price \$24.00 per year Canada \$25.00 per year
Foreign \$25.00 per year

ESTABLISHED 1896

THEODORE E. WALSH, M.D.
EDITOR

222 PINE LAKE ROAD, COLLINSVILLE,
ILLIOIS 62234

Please mention *The Journal of Laryngology and Otology* when replying to advertisements

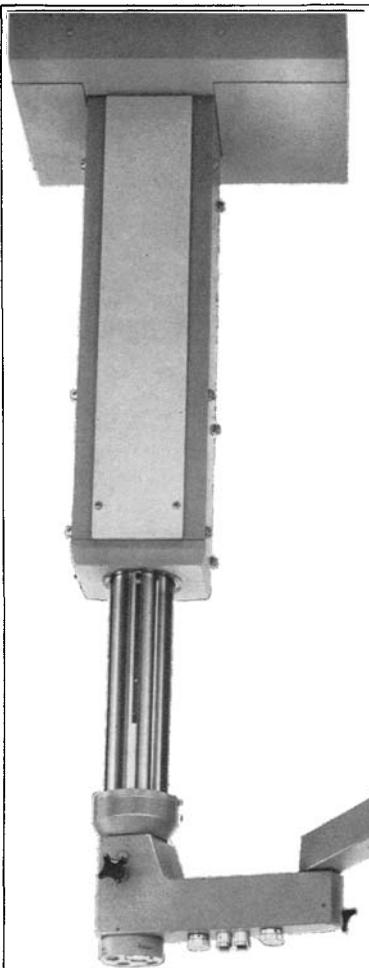

New from Zeiss Ceiling Suspension Unit

Suitable for new and existing Theatres.

All seven Zeiss Operating Microscopes can be attached to it.


Avoids the need for large floor stands.

Automatic electro-hydraulic operation by hand or foot controls.

Two telescoping speeds – one for rapid positioning, one for precision fine focusing of the microscope.

The illustration shows the Ceiling Unit carrying the new Zeiss Operating Microscope 6.

To be shown at the
3rd British Academic Conference
Otolaryngology, Edinburgh, July.

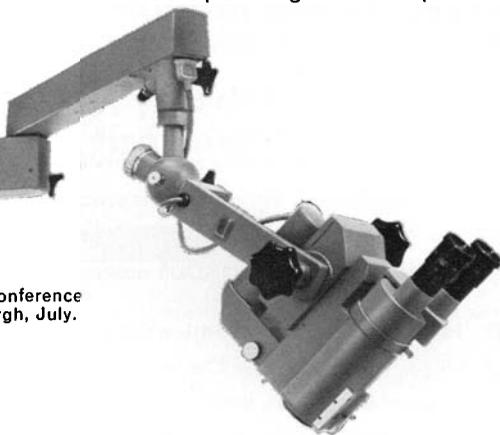


ZEISS

The great name in optics



Degenhardt

Demonstrations can be arranged, full details from Degenhardt and Co Ltd
Carl Zeiss House
31/36 Foley Street
London W1P 8AP
01-636 8050
Cable: Zeissag London
Telex: 24300

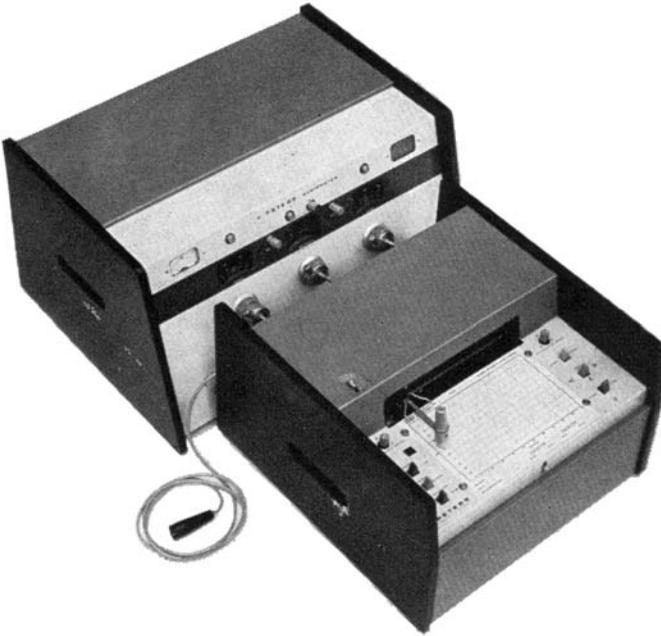

PETERS CLINIC AUDIOMETERS AND BÉKÉSY
ARE THE IDEAL TOOLS FOR MORE ADVANCED AUDIOMETRY


The Audiometers offer :

- Two continuously variable attenuators accurate to 1 db.
- SISI Test (built-in) and automatic alternate loudness balance switching.
- Maximum attenuation of 120 db for loudness discomfort level tests.
- Narrow band SYNCHRONOUS masking (a new semi-automatic masking technique).
- Full speech test facilities with white noise masking.
- Plug-in circuit boards and operator output checks.
- Conversion to a true BÉKÉSY AUDIOMETER at will.
- Extra features not listed are offered by the AP/6 compared to the AP/5 AUDIOMETER.

write for full details to:


ALFRED PETERS AND SONS LTD
GELL STREET SHEFFIELD 3

Please mention *The Journal of Laryngology and Otology* when replying to advertisements

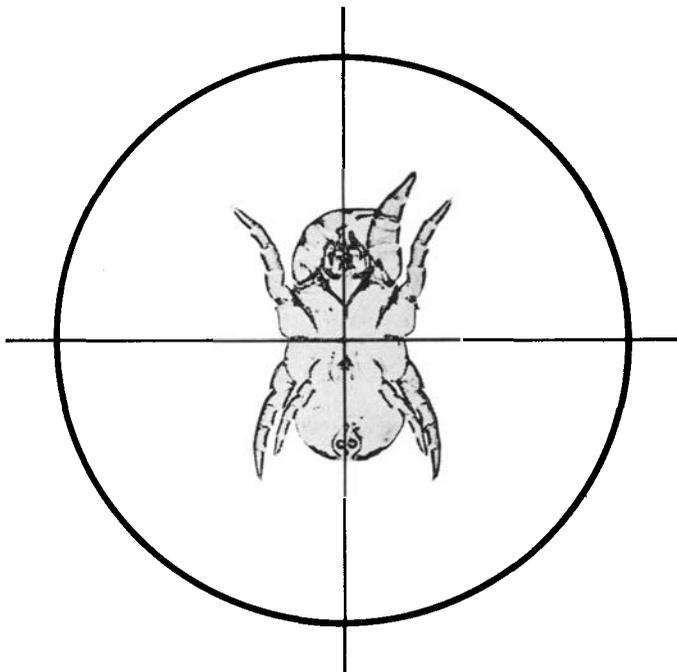

you always knew
the house dust mite
was the target...

**unfortunately, you didn't have a
bullet to fire-until now!**



The house dust mite (*Dermatophagoides* sp.) has been known as an important factor in house dust allergy for some time now. With the aid of the Dome glycerinated extract of house dust mite, many doctors have shown that allergic symptoms, of

previously unknown cause in some patients, may in fact be due to the house dust mite. For the first time, it is now possible to offer these patients a course of hyposensitisation using ...

mite fortified house dust

an addition to the range of

Allpyral

allergen extracts


Full information is available on request



DOME LABORATORIES, DIVISION OF MILES LABORATORIES LTD
STOKE COURT, STOKE POGES, SLOUGH, BUCKS. TEL: FARNHAM COMMON 2151



ALLPYRAL is a trademark
DM 393

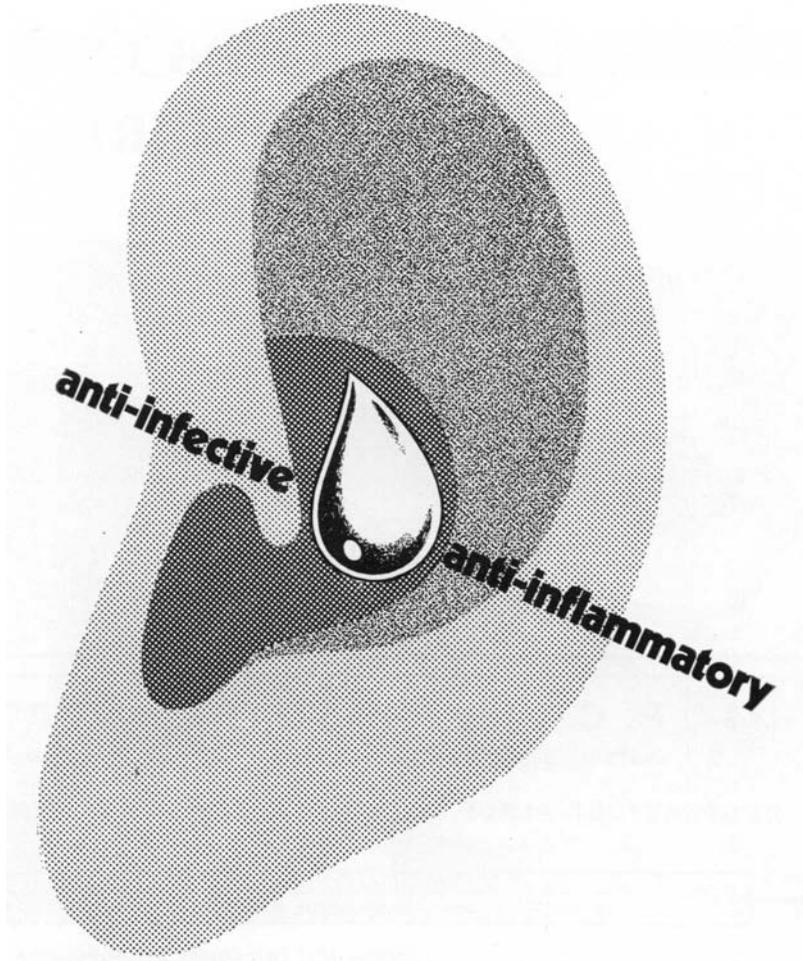

the drop that soothes and clears infected ears

soothes by reducing inflammation with hydrocortisone
clears by rapidly destroying virtually all bacteria commonly
found in ear infections

*
OTOSPORIN drops contain polymyxin B sulphate, neomycin sulphate
and hydrocortisone in a bland suspension designed to facilitate penetration.
Supplied in dropper bottles of 5 ml. Full information is available on request.

*Trade Mark

OTOSPORIN



Burroughs Wellcome & Co.
(The Wellcome Foundation Ltd.) Dartford, Kent

Please mention *The Journal of Laryngology and Otology* when replying to advertisements