

INFECTION CONTROL



EDITORIAL

The Role of Epidemiology in Medical Education

Robert Waldman, MD

ORIGINAL ARTICLES

Tuberculosis in Hospital Personnel

Loraine E. Price, BSN, CIC; William A. Rutala, PhD, MPH; Gregory P. Samsa, MS

A Hepatitis B Vaccination Program in a Community Teaching Hospital

Myron J. Tong, MD, PhD; Ann M. Howard, MD; Gary C. Schatz, MD; Mark A. Kane, MD; Deborah A. Roskamp; Ruth L. Co; Cissy Boone

Emergence of Coagulase Negative Staphylococci as Major Nosocomial Bloodstream Pathogens

Richard I. Stillman, MD; Richard P. Wenzel, MD, MSc; Leigh G. Donowitz, MD

Intravenous Tubing Containing Burettes Can Be Safely Changed at 72 Hour Intervals

David R. Snyderman, MD; Maureen Donnelly-Reidy, BSN, RN; Linda K. Perry, CLS/M (NCA); William J. Martin, PhD


SPECIAL SECTIONS

Clinical Pharmacology of Antibiotics: Review of the 4-Quinolones

Mark Eggleston, PharmD; Soon-Young Park, PharmD

Now Available . . .
Sporicidin® brand
Disinfectant Spray

Disinfect Scopes Safely and Completely in just 10 Minutes

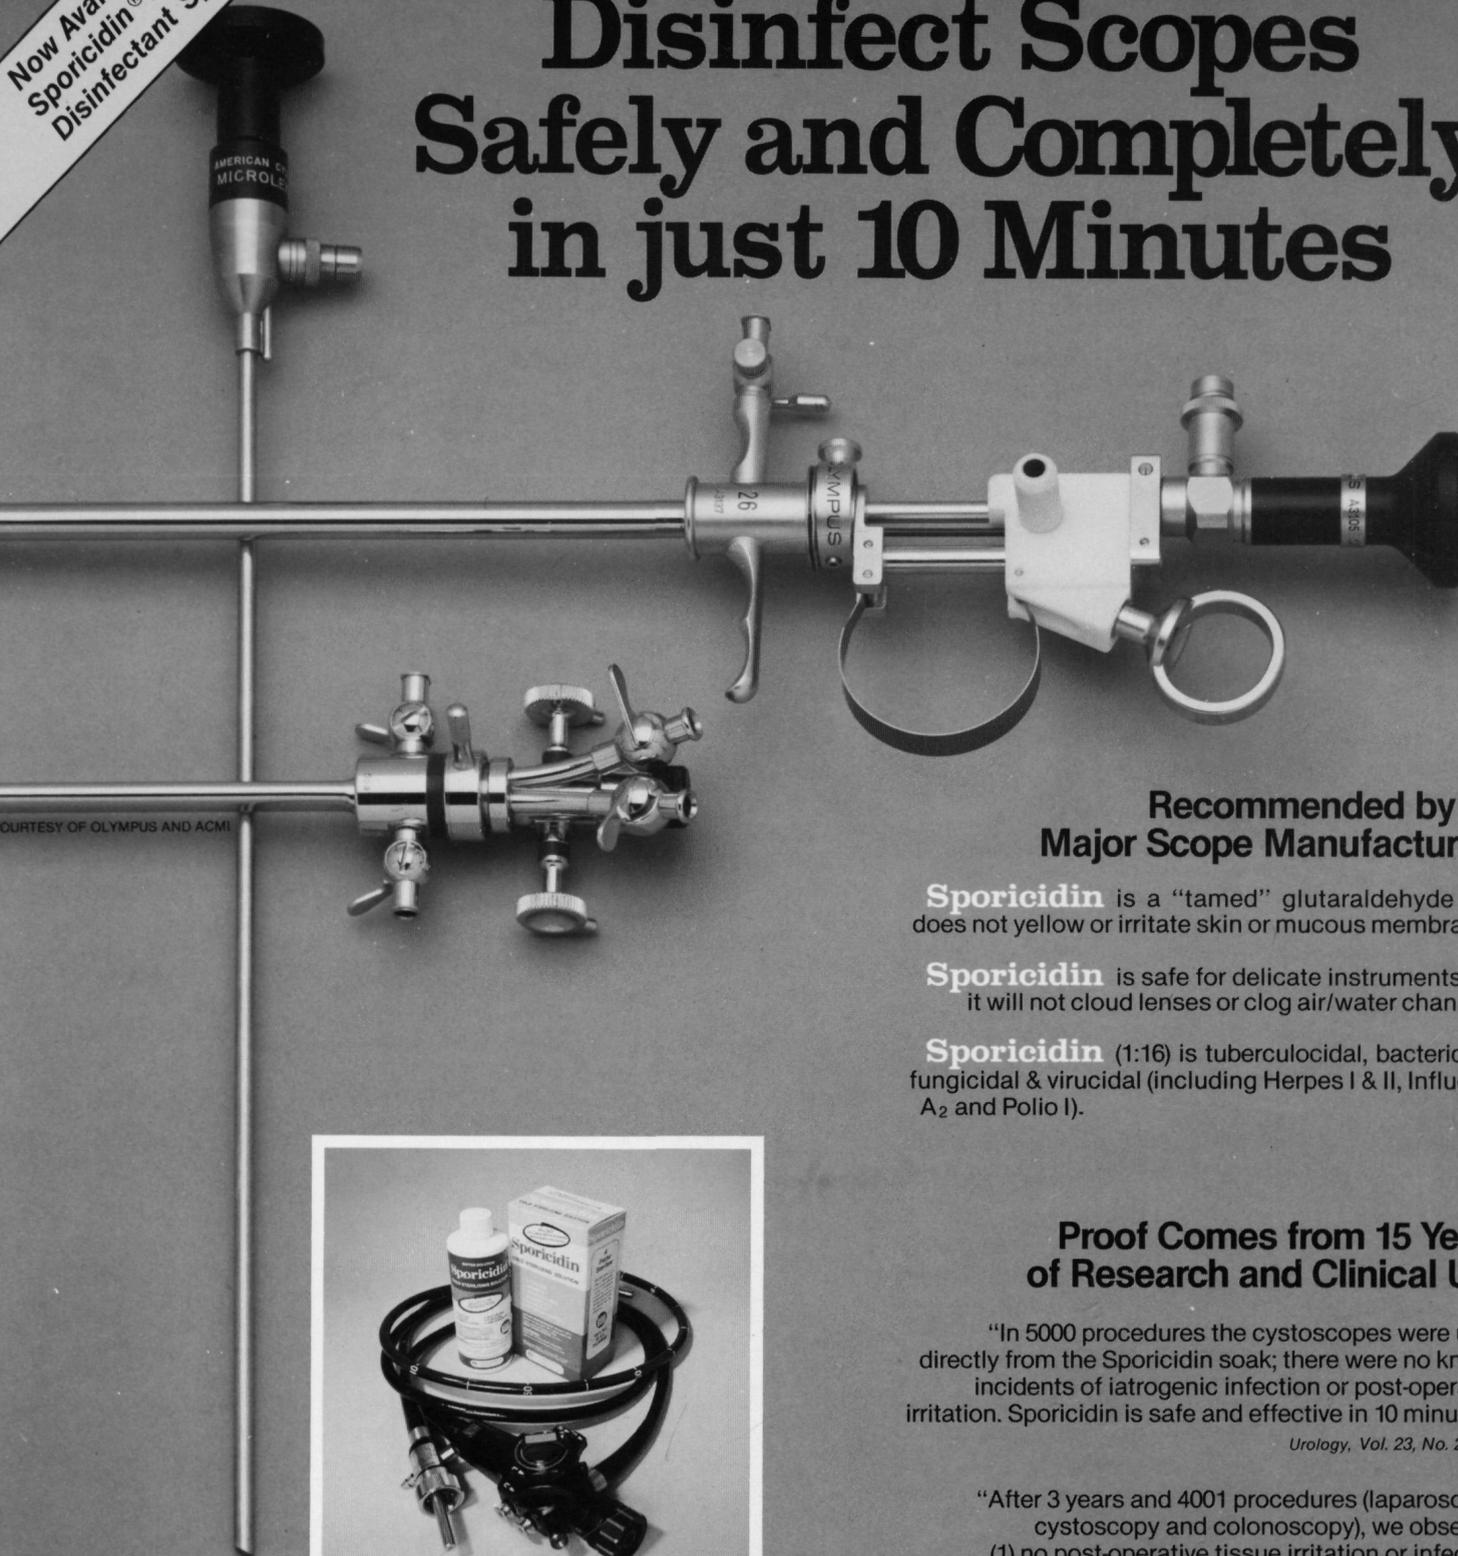

COURTESY OF OLYMPUS AND ACMI

Recommended by All Major Scope Manufacturers

Sporicidin is a "tamed" glutaraldehyde that does not yellow or irritate skin or mucous membranes.

Sporicidin is safe for delicate instruments and it will not cloud lenses or clog air/water channels.

Sporicidin (1:16) is tuberculocidal, bactericidal, fungicidal & virucidal (including Herpes I & II, Influenza A₂ and Polio I).

Proof Comes from 15 Years of Research and Clinical Use

"In 5000 procedures the cystoscopes were used directly from the Sporicidin soak; there were no known incidents of iatrogenic infection or post-operative irritation. Sporicidin is safe and effective in 10 minutes."

Urology, Vol. 23, No. 2, 1984

"After 3 years and 4001 procedures (laparoscopy, cystoscopy and colonoscopy), we observed
(1) no post-operative tissue irritation or infection
(2) no lens clouding or endoscope damage
(3) preferred by our staff."

*Journal Of The Operating Room
Research Institute, Vol. 3, No. 8, 1983*

"Sporicidin . . . was both more stable and more active against test spores than . . . Cidex and Cidex-7."

Infection Control, Vol. 1, No. 2, 1980

These and other studies available upon request.

Sporicidin[®]
COLD STERILIZING SOLUTION
An exclusive glutaraldehyde formula



*Hands
that serve deserve
the best*

HIBICLENS[®]

Antiseptic/antimicrobial
skin cleanser



STUART PHARMACEUTICALS
Division of ICI Americas Inc.
Wilmington, Delaware 19897

© 1986 ICI Americas Inc.

<https://doi.org/10.1017/S0195941700067197> Published online by Cambridge University Press

INFECTION CONTROL®

Table of Contents

EDITORIAL

- The Role of Epidemiology in Medical Education** 95
Robert Waldman, MD

ORIGINAL ARTICLES

- Tuberculosis in Hospital Personnel** 97
Loraine E. Price, BSN, CIC; William A. Rutala, PhD, MPH;
Gregory P. Samsa, MS

- A Hepatitis B Vaccination Program in a Community Teaching Hospital** 102
Myron J. Tong, MD, PhD; Ann M. Howard, MD; Gary C. Schatz, MD;
Mark A. Kane, MD; Deborah A. Roskamp; Ruth L. Co; Cissy Boone

- Emergence of Coagulase Negative Staphylococci as Major Nosocomial Bloodstream Pathogens** 108
Richard I. Stillman, MD; Richard P. Wenzel, MD, MSc;
Leigh G. Donowitz, MD

- Intravenous Tubing Containing Burettes Can Be Safely Changed at 72 Hour Intervals** 113
David R. Snyderman, MD; Maureen Donnelly-Reidy, BSN, RN;
Linda K. Perry, CLS/M (NCA); William J. Martin, PhD

SPECIAL SECTIONS

- Clinical Pharmacology of Antibiotics: Review of the 4-Quinolones** 119
Mark Eggleston, PharmD; Soon-Young Park, PharmD

DEPARTMENTS

- | | | | |
|--------------------------------|-----|-------------------------------|-----|
| Information for Authors | 85 | Calendar of Events | 129 |
| Letters to the Editor | 90 | Classified Marketplace | 132 |
| Book Reviews | 127 | | |

The ideas and opinions expressed by contributing authors do not necessarily reflect those of the editors or publisher.

Publisher: Infection Control (ISSN-0195-9417) is published monthly by SLACK Incorporated, 6900 Grove Road, Thorofare, New Jersey 08086. Telephone: (609) 848-1000.

Copyright 1987: All rights reserved. No part of this publication may be reproduced without written permission from the publisher.

Subscriptions. Requests should be addressed to the publisher (except Japan). In Japan, contact Woodbell Scope Incorporated, Mansui Bldg., 9-18, Kanda Surugadai 2-chome, Chiyoda-ku, Tokyo 101, Japan. Subscription rates in the US and possessions: Individual: One year—\$40.00; Two years—\$66.00; Three years—\$94.00. Institutional: One year—\$55.00; Two years—\$92.00; Three years—\$128.00; Canada: \$15.00 additional each year; all other countries: \$25.00 additional each year. Single copies of current issues may be obtained for \$7.00, United States and possessions; \$13.00 all other countries.

Change of address: Notice should be sent to the publisher six weeks in advance of effective date. Include old and new addresses with zip codes. The publisher cannot accept responsibility for undelivered copies. Second-class postage is paid at Thorofare, New Jersey 08086. **Postmaster:** Send address changes to SLACK Incorporated, 6900 Grove Road, Thorofare, NJ 08086.

As of Volume 1, Number 1, INFECTION CONTROL is listed in *Index Medicus*, *Current Contents—Clinical Practice*, *Hospital Literature Index*, and *Cumulative Index to Nursing and Allied Health Literature*.

EDITOR

Richard P. Wenzel, MD, MSc
Iowa City, Iowa

SENIOR ASSOCIATE EDITOR

William Schaffner, MD
Nashville, Tennessee

ASSOCIATE EDITORS

Sue Crow, MSN, RN
Shreveport, Louisiana

John E. McGowan, Jr., MD
Atlanta, Georgia

Dennis G. Maki, MD
Madison, Wisconsin



SLACK Incorporated
6900 Grove Road
Thorofare, New Jersey 08086

Publisher
Richard N. Roash

Editorial Director
Donna Carpenter

Editorial Coordinator
Sandra L. Patterson

Assistant Editor
Dawn A. Zwick

Circulation Manager
Kevin J. Fenton

Advertising Manager
Randall Roash

**Advertising
Sales Representative**
Wayne M. McCourt

**Advertising Sales
Coordinator**
Betty Martz

**Classified
Advertising Representative**
Donna M. Coles

EDITORIAL OFFICES

C41 General Hospital
University of Iowa Hospitals and Clinics
Iowa City, Iowa 52242
(319) 356-0463

William J. Hausler, Jr., PhD
R. Michael Massanari, MD, MS
Michael Pfaller, MD

Managing Editor
Marikay Klein

EDITORIAL ADVISORY BOARD

Robert C. Aber, MD
Hershey, Pennsylvania

Paul Arnow, MD
Chicago, Illinois

Charles S. Bryan, MD
Columbia, South Carolina

John P. Burke, MD
Salt Lake City, Utah

Mary Castle, MPH, RN
Berkeley, California

Marie B. Coyle, PhD
Seattle, Washington

Burke A. Cunha, MD
Mineola, New York

Richard E. Dixon, MD
Trenton, New Jersey

Leigh G. Donowitz, MD
Charlottesville, Virginia

Mark Eggleston, PharmD
Washington, DC

Harvey A. Elder, MD
Loma Linda, California

Bruce Farber, MD
Pittsburgh, Pennsylvania

Martin S. Favero, PhD
Atlanta, Georgia

Peter C. Fuchs, MD, PhD
Portland, Oregon

Richard A. Garibaldi, MD
Farmington, Connecticut

Angella Goetz, MEd, RN
Pittsburgh, Pennsylvania

Donald A. Goldmann, MD
Boston, Massachusetts

Dieter H.M. Gröschel, MD
Charlottesville, Virginia

Peter A. Gross, MD
Hackensack, New Jersey

Karen Hadley, MPH, RN
New Orleans, Louisiana

David K. Henderson, MD
Bethesda, Maryland

Peter N.R. Heseltine, MD
Los Angeles, California

Cyrus C. Hopkins, MD
Boston, Massachusetts

Allen B. Kaiser, MD
Nashville, Tennessee

Donald L. Kaiser, DrPH
Charlottesville, Virginia

Elaine Larson, PhD
Cabin John, Maryland

Harold Laufman, MD, PhD
New York, New York

Barbara McArthur, PhD, RN
Detroit, Michigan

Rob Roy MacGregor, MD
Philadelphia, Pennsylvania

C. Glen Mayhall, MD
Richmond, Virginia

Patti J. Miller, MS
Charlottesville, Virginia

Harry C. Nottebart, Jr., JD, MD
Richmond, Virginia

James E. Peacock, Jr., MD
Winston-Salem, North Carolina

Frank S. Rhame, MD
Minneapolis, Minnesota

William A. Rutala, PhD, MPH
Chapel Hill, North Carolina

William E. Scheckler, MD
Madison, Wisconsin

Walter E. Stamm, MD
Seattle, Washington

Charles W. Stratton, MD
Nashville, Tennessee

Richard L. Sweet, MD
San Francisco, California

George H. Talbot, MD
Philadelphia, Pennsylvania

Timothy R. Townsend, MD
Baltimore, Maryland

James Veazey, MD
Albany, New York

FOREIGN ADVISORY BOARD

Graham Ayliffe, MD, FRCPath.
Birmingham, England

Professor G. Berencsi
Szeged, Hungary

David Birnbaum, MPH
Sidney, British Columbia, Canada

Professor Jaap Dankert
Groningen, Netherlands

Professor Dr. F. Daschner
Freiburg, West Germany

Lars O. Kallings, MD
Stockholm, Sweden

Professor W.B. Kędzia
Sieroca, Poland

Professor A.P. Krasilnikov
Minsk, USSR

Professor Dr. W. Marget
Munich, West Germany

Jonathan L. Meakins, MD,
FRCSC, FACS
Montreal, Canada

Bertil Nyström, MD
Huddinge, Sweden

Ian Phillips, MA, MD, MRCPath.
London, England

Samuel Ponce de Leon, MD
Mexico City, Mexico

Hans Reber, MD
Basel, Switzerland

Professor Gerald Reybrouck
Leuven, Belgium

Manfred L. Rotter, MD, DipBact
Vienna, Austria

Theodore Sacks, MD
Jerusalem, Israel

Dr. Bernhard M. Thimm
Federal Republic of Germany

Professor Dr. med. H.P. Werner
Mainz, West Germany

Professor Dr. W. Weuffen
Greifswald, German Democratic
Republic


Important steps in reducing the risk of contamination in tracheostomy patients.

Throw contamination away! That's what every health care professional wants to do in treating tracheostomy patients. And that desire is closer to reality with Shiley's Disposable Inner Cannula (DIC) system of tracheostomy tubes.

Since the DIC was first introduced, doctors, nurses and therapists have accepted it as a significant advance in reducing the risk of contamination and infection, as well as a time and cost saver.¹ Tracheostomy care procedures can be simplified and trach care kits can be eliminated.



DIC is used with all Shiley disposable cannula tracheostomy tubes.

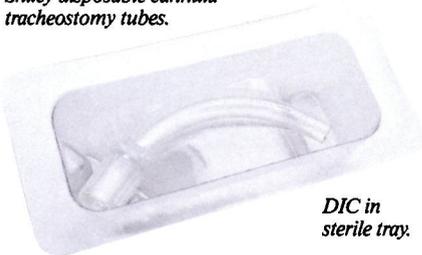


DIC in sterile tray.

To realize the benefits of the disposable inner cannula, the health care professional simply needs to follow these four important steps:

Step 1—Remove the used inner cannula, employing aseptic procedures, by firmly pinching the clamps of the snap-lock connector and gently pulling back from the tracheostomy tube. The professional should note the size of the tube for correct DIC replacement.

Step 2—Important! After determining that the inner cannula is indeed a disposable type (and not a reusable inner cannula with a twist lock), discard the DIC in an appropriate disposal container. **Remember, do not clean, resterilize, or reuse the DIC.**

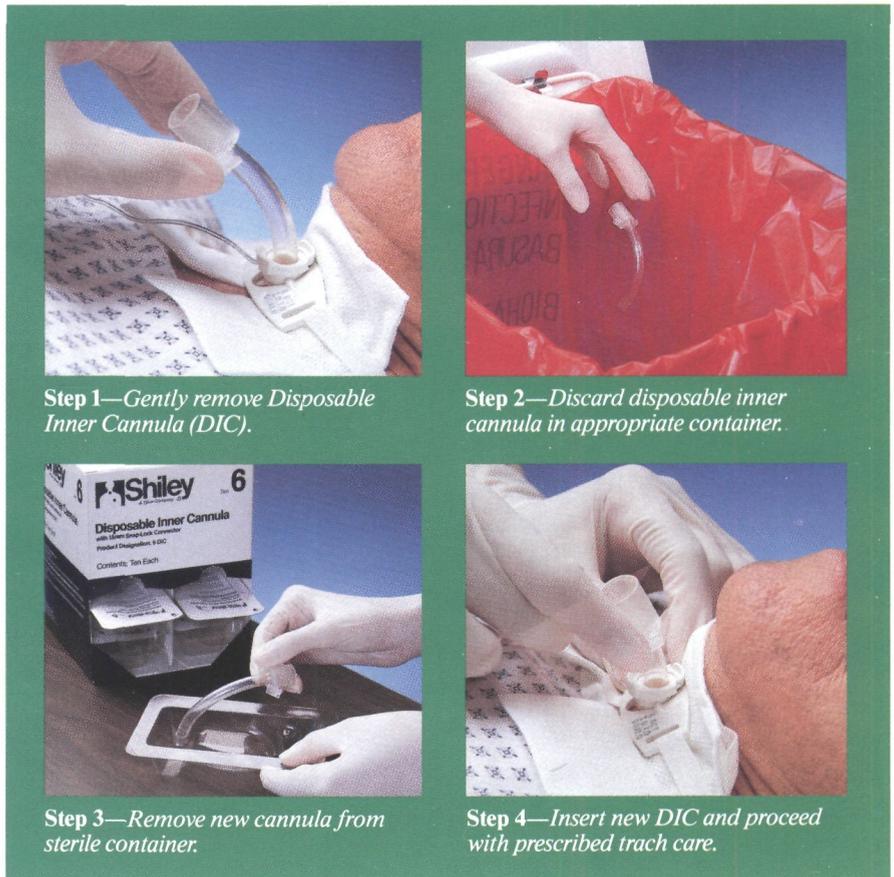

Step 1—Gently remove Disposable Inner Cannula (DIC).

Step 2—Discard disposable inner cannula in appropriate container.

Step 3—Remove new cannula from sterile container.

Step 4—Insert new DIC and proceed with prescribed trach care.

Step 3—Remove the correct size DIC from its sterile container by the pinch clamps of the snap-lock connector using aseptic technique.

Step 4—Still using aseptic technique, insert the new DIC, securely snapping both sides of the connector, and proceed with hospital-prescribed trach care. The sterile tray from the DIC makes a convenient basin for stoma care.

So, take a **big step** in reducing the risk of contamination and infection—by throwing away the used disposable inner cannula. For more information, and for details on our informative video program about tracheostomy care, contact your Shiley Technical Representative at (800) 233-8969 or write to Shiley Incorporated, 17600 Gillette Avenue, Irvine, CA 92714-5751 U.S.A., Tel: (714) 250-

0500, (800) 854-3683, Cable: SHILEYINC IRIN, Telex: 68-5585. Shiley-Europe, Staines House, 158-162 High Street, Staines, TW18 4AZ, ENGLAND, Tel: (44) 784-61533, Telex: 919851 PFHPPGS-G. Shiley Canada, 251 Bartley Drive, Toronto, Ontario, M4A-2N7 CANADA, Tel: (416) 752-9990, Telex: 06963811.



¹Sue Crow, R.N, MSN, "Disposable Tracheostomy Inner Cannula," *Infection Control*, Vol. 7, No. 5, 1986, pp. 285-286.

For detailed information describing intended use, warnings, precautions and contraindications, refer to the instructions provided with each device or contact the Shiley corporate office. © Shiley Incorporated, 1987. All rights reserved. 086R211 (1/87)